

THE MEASURABLE DIFFERENCE.



DEWETRON

▼

OXYGEN TRAINING > RECORDER








- > Placing a recorder on the screen
- > Channel assignment
- > Changing X-axis scaling
- > Changing Y-axis scaling
- > Sync'ing X-axes of several recorder
- > Cloning a recorder
- > Using A/B cursors
- > DejaView



PLACING A RECORDER ON THE SCREEN

- 1 Drag and drop a Recorder to the measurement screen
- 2 Adjust the size by grabbing the Recorder in one of the grey corners
- 3 Change the position by grabbing the Recorder somewhere except the grey corners

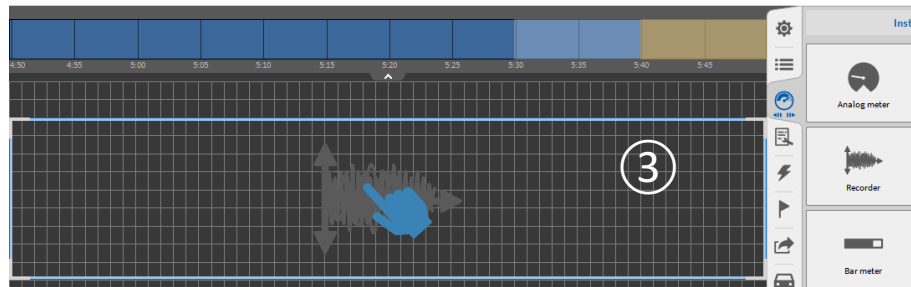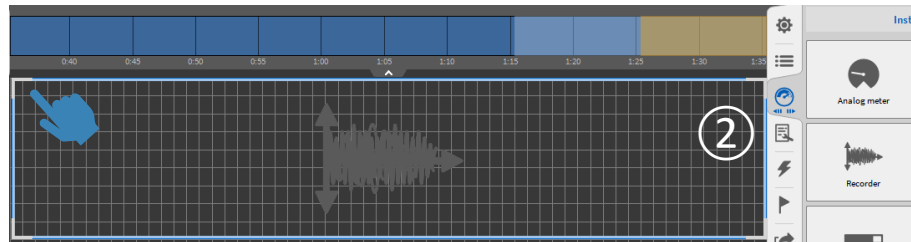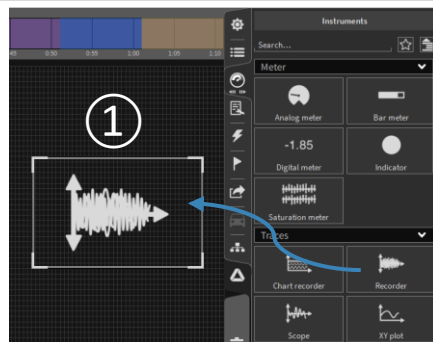

CHANNEL ASSIGNMENT




DEWETRON

① Go to the Channel List and select the Channels to be assigned from the List

Up to 40 channels can be assigned to one Recorder

Recorder must be selected here
(blue box around the Recorder)



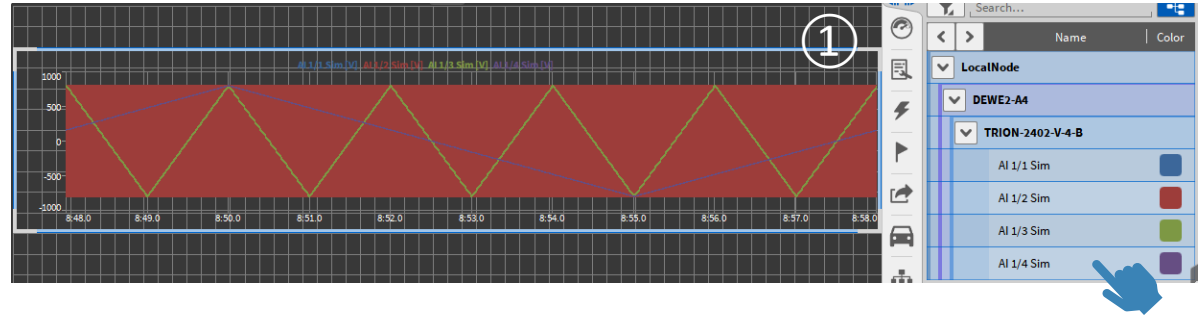




DEWETRON

CHANGING THE X-AXIS SCALING

- 1 Press on the X-Axis for 2 seconds
- 2 Move the mouse into the Recorder and use the scroll wheel
- 3 Time scaling can be changed between Absolute and Relative time in the Recorder properties

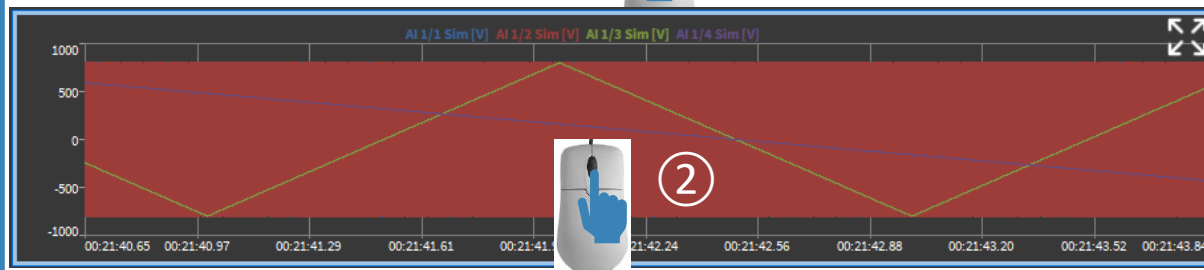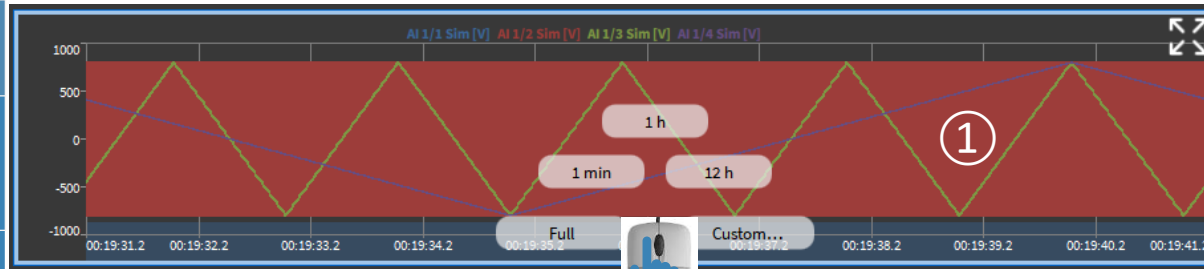

Design Mode must be deactivated for these actions (no grey grid on the screen)




A click on the right mouse button will revert the applied zooming actions one by one






DEWETRON

CHANGING THE X-AXIS SCALING CONT'D

④ Scrolling the mouse wheel will zoom the X-axis
Pressing the *SHIFT* button will enlarge the zoom steps

⑤ In *Freeze* (see ) or *PLAY* mode, the time axis can be zoomed by pressing the right mouse button

⑥ A box zoom is available as well

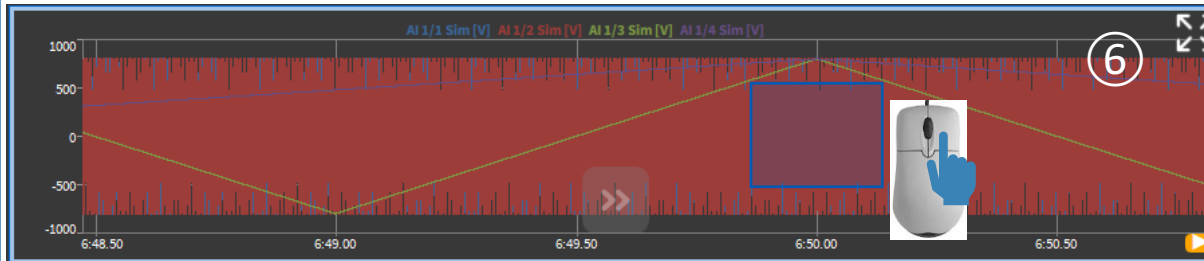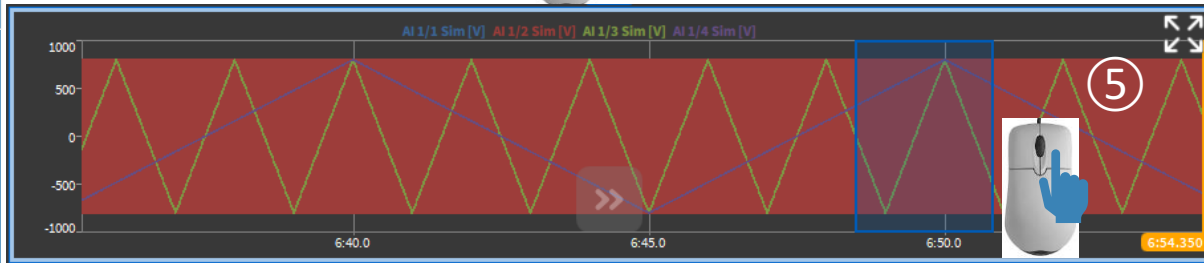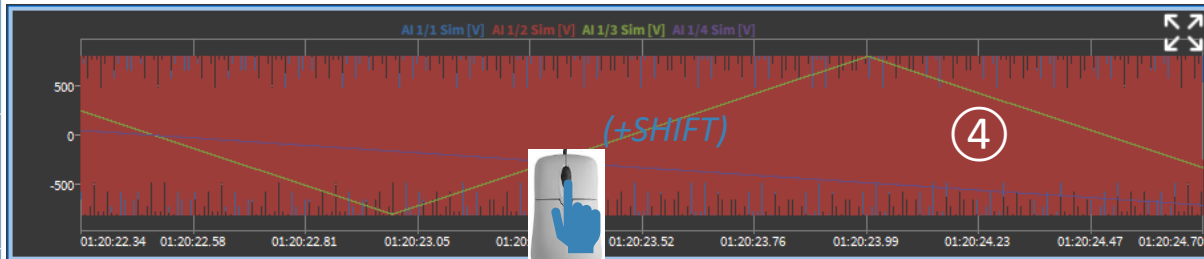

Design Mode must be deactivated for these actions (no grey grid on the screen)








DEWETRON

© DEWETRON GmbH | January 24

CHANGING THE Y-AXIS SCALING

- ① Press in the middle of the Y-axis for 2 seconds
- ② Press on the minimum or maximum value on the Y-axis
- ③ Y-axis scaling can be edited for all Channels in the Recorder Properties
- ④ Y-axis scaling can be edited channel-wise in the Recorder Properties
- ⑤ Y-axis can be automatically scaled to actually displayed minimum/maximum in the Recorder properties

Design Mode must be deactivated for these actions (no grey grid on the screen)

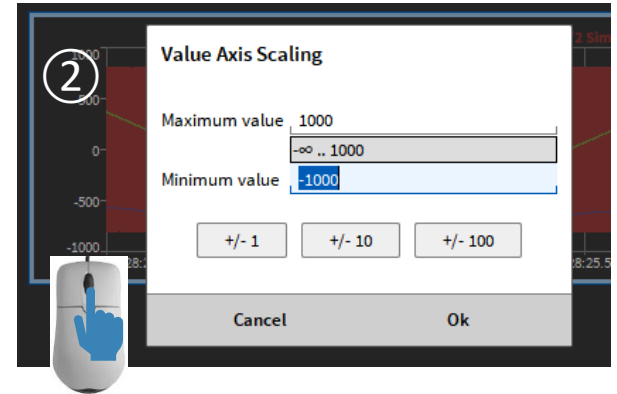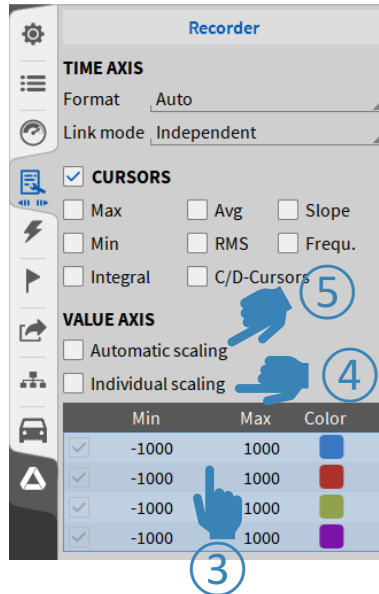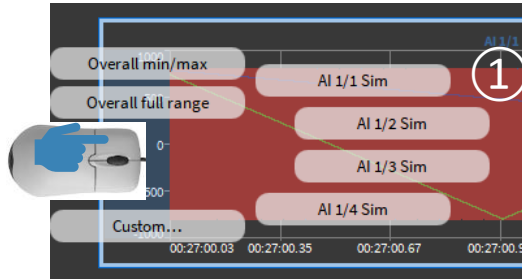

A click on the right mouse button will revert the applied zooming actions one by one





DEWETRON

© DEWETRON GmbH | January 24

CHANGING THE Y-AXIS SCALING CONT'D

- ⑥ Box zoom is available when pressing the right mouse button on the Recorder
- ⑦ Moving the mouse wheel while pressing **CTRL** will zoom the Y-axis in and out

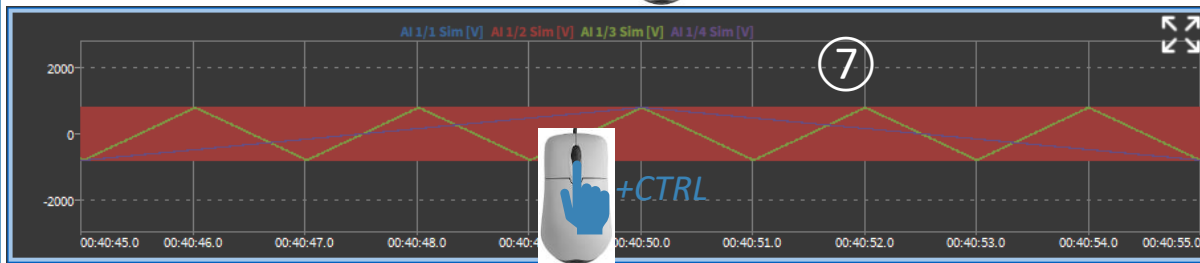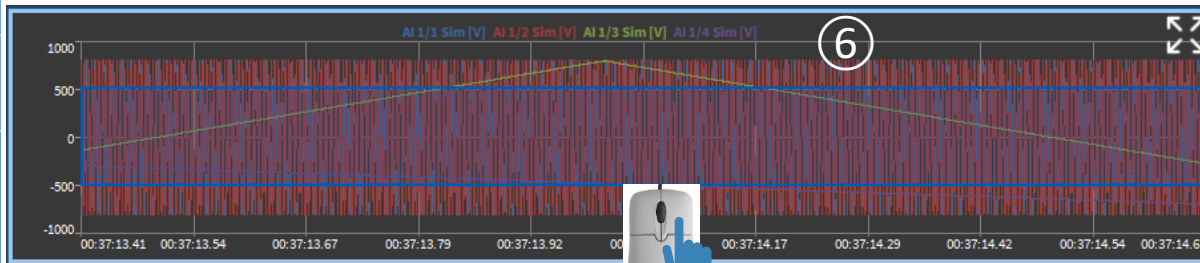

Design Mode must be deactivated for these actions (no grey grid on the screen)



A click on the right mouse button will revert the applied zooming actions one by one




DEWETRON

SYNC'ING THE X-AXES OF SEVERAL RECORDERS

- ① If Recorders are placed below each other, the X-axes will be locked and zooming actions will be applied to all Recorders
- ② *Lck* in the lower left corner of the Recorder will indicate that they are locked

*Design Mode must be deactivated for these actions
(no grey grid on the screen)*

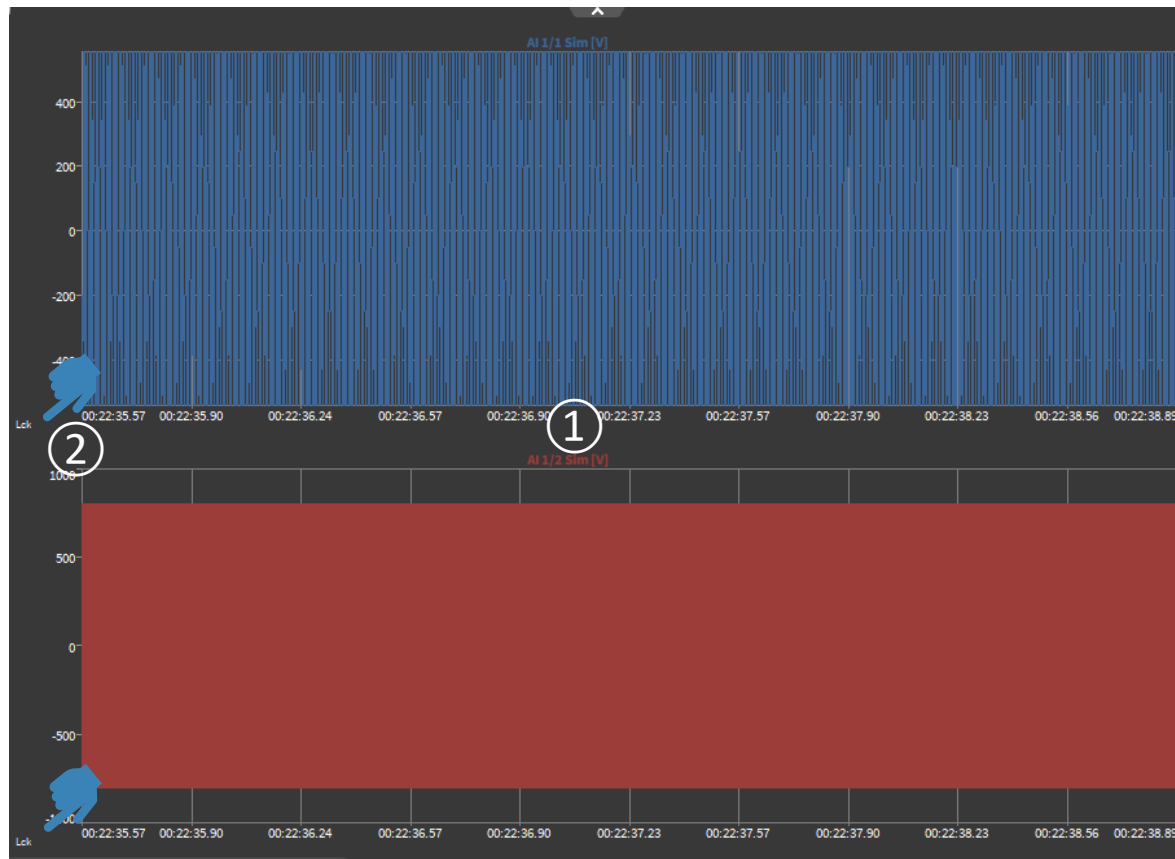

CLONING RECORDERS




DEWETRON

- 1 A Recorder can be cloned by *Copy-and-Paste*





RECORDER & A/B CURSORS

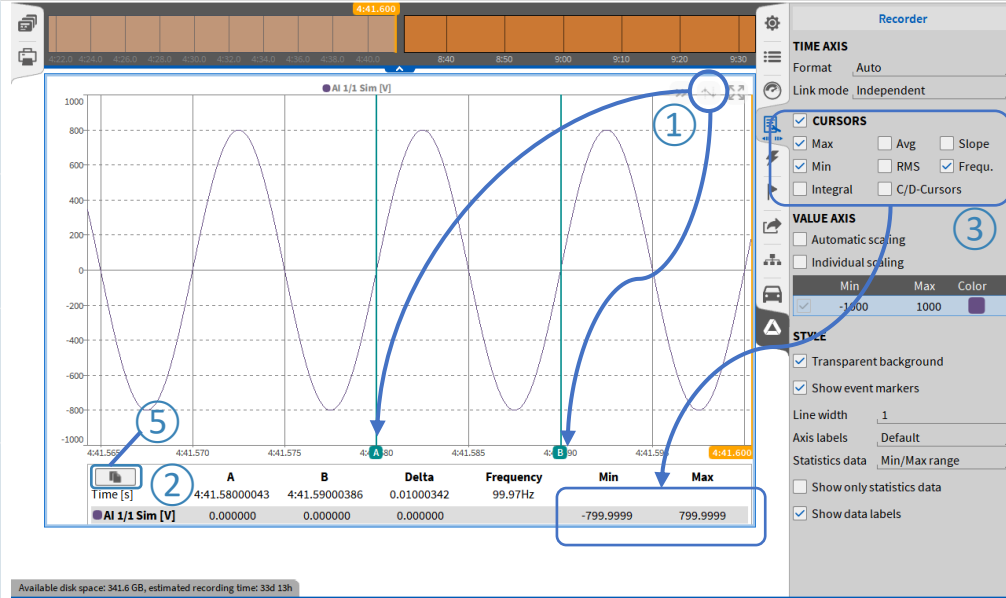

Available disk space: 341.6 GB, estimated recording time: 33d 13h

① Activate the Cursors with the *Cursor* button
The A/B cursors can be moved with the mouse

② Actual position and signal value for all signals in the Recorder can be seen in the table below


③ Certain Statistics for the signal between both cursors can be selected in the Recorder Properties

④ A/B cursors can be renamed in the popup, which opens with a click on the cursor name. Deactivating and activating cursors again keeps the individual name stored and cursors of several Recorders can be renamed individually

Remark: A and B cursor can be moved simultaneously when pressing *shift*. This is also true for C/D cursor.

Remarks:

- Cursors are only applicable in Freeze and PLAY mode
- Cursors can be activated for Recorder, Chart Recorder and Scope

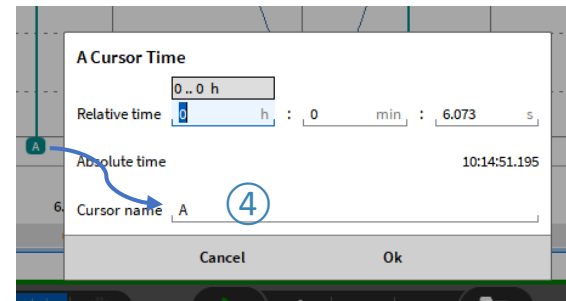




DEWETRON

RECORDER COPY CURSOR VALUES TO CLIPBOARD

① With a left click with the mouse on this button, the A/B cursor values can be copied to the clipboard and pasted, for example, in an Excel list. This operation also works with the key combination "CTRL" + "C" if you have selected the recorder instrument.

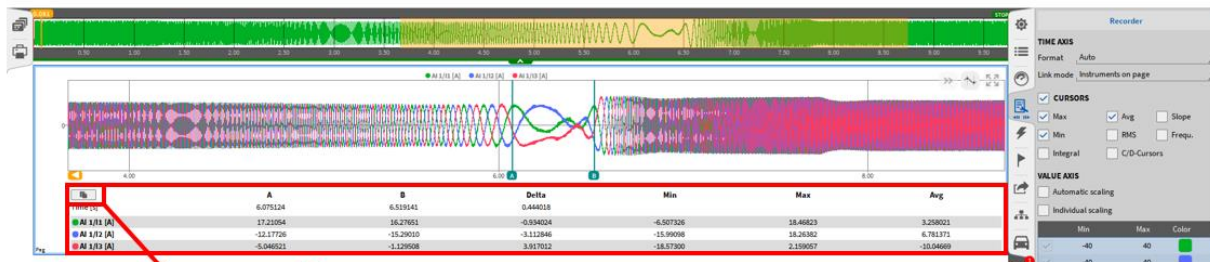


The screenshot shows an Excel spreadsheet with the following data:

Channel	Unit	A	B	Delta	Min	Max	Avg
Time	s	6,07512376	6,51914134	0,44401758			
AI 1/11	A	17,210537	16,2765131	-0,93402391	-6,50732556	18,4682285	3,25802063
AI 1/12	A	-12,1772583	-15,2901039	-3,11284561	-15,990983	18,2638227	6,78137147
AI 1/13	A	-5,04652053	-1,12950809	3,91701245	-18,5729992	2,15905679	-10,046691



RECORDER & LABELS

- ① Activate the labels with the „Data Label“ button. It is now possible to display the labels in the recorder at the position selected with the mouse. The fixed setting of several labels is only possible for recorded measurements.
- ② If activated, all set labels will be displayed, if deactivated the set labels will be hidden
- ③ Labels can be deleted by pressing „X“ on the right top of the label.

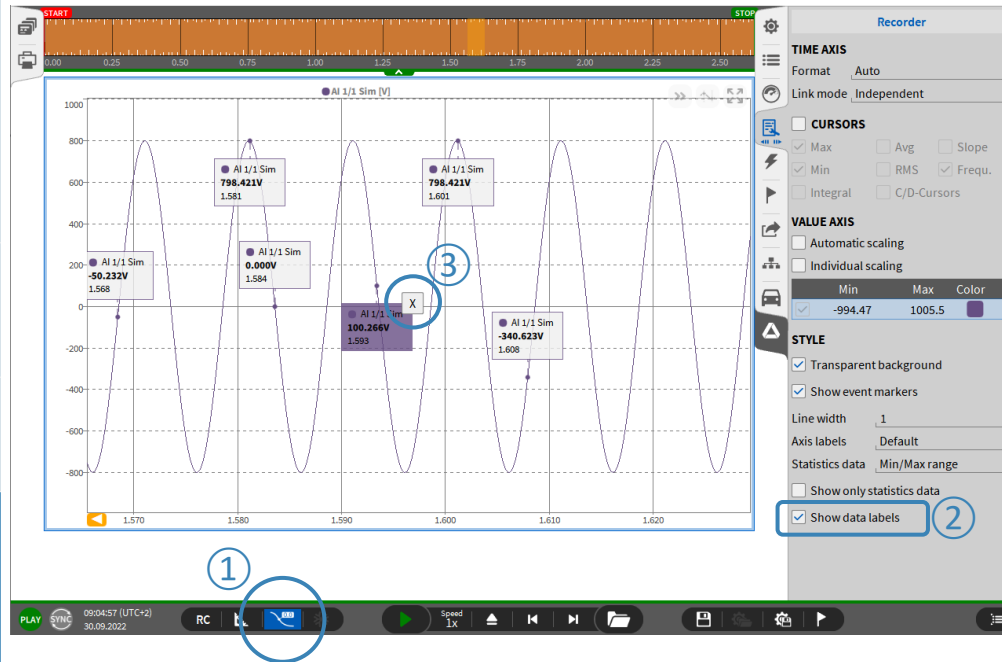

Remarks:

- If ① is deactivated the mouseover labels will be disabled. The inserted labels will be visible.
- If ② is deactivated all labels of this recorder will be invisible



DEWETRON

© DEWETRON GmbH | January 24

DEJAVIEW – REVIEW DATA WHILE RECORDING

- 1 Select a Recorder and move the data to the left
- 2 Go back until data of interest is reached; The mouse wheel, box zoom with right click and adjustment of axes scaling can be used to zoom into the data
The orange box in the Overview bar marks the actual position in the data file
- 3 Enable A/B cursors for detailed data analysis; Cursor position can be changed with the mouse
- 4 Go to the Recorder properties (double click on the Recorder or open Properties menu on the right hand side) for measuring predefined values between both cursors
- 5 When finished press the >> button to jump back to the actual data

The screenshot shows the DEWETRON software interface with two panels illustrating the steps. The top panel shows step 1: a blue arrow points to the left in the overview bar, and a blue circle '1' is next to a hand icon. The bottom panel shows step 2: a blue circle '2' is in the overview bar, and a blue circle '3' is on the zoom controls. Step 3 shows two vertical cursors labeled 'A' and 'B' on the waveform. Step 4 shows the 'Recorder' properties panel with 'Cursors' and 'Value Axis' options checked. Step 5 shows a blue circle '5' on the '>>' button in the zoom controls. A table at the bottom of the interface displays the following data:

Time [s]	A	B	Delta	Min	Max	Avg
0:37.5032905	0:37.5032905	0:37.5288188	0.0255283	0.548296	0.870967	0.641214
0:37.5032905	0.634799	0.562679	-0.072120	0.548296	0.870967	0.641214